

AUTOMATED LOW-LEVEL TRITIUM IN WATER MONITOR REAL TIME CONTINUOUS

Model ~ NexTritium-H₂O

FEATURES:

- LOW LEVEL TRITIUM
- SENSITIVE TO 0.2 $\mu\text{Ci/l}$ Tritium
- REAL TIME – AUTOMATIC
- EXCELLENT LONG-TERM STABILITY
- MEETS EPA DRINKING WATER LEVELS
- CONTINUOUS MONITORING
- NOT INFLUENCED BY OTHER NUCLIDES
- NO LIQUID SCINTILLANT REQUIRED
- EASY CALIBRATION
- NEW STATISTICAL SIGNIFICANCE DISPLAY
- RUGGED,
- MOUNTED: CASTER, SKID, or BENCH TOP
- IP 42



NexTritium-H₂O
Electronics



Two Pairs of Matched
Photo Multiplier
Tubes

APPLICATION:

- MEETS EPA DRINKING WATER LEVELS
- MONITOR LEAKS IN CANDU TYPE REACTORS MONITOR TRITIUM
- CONTAMINATION IN GROUND WATER.
- MONITOR LABORATORY OR PLANT LIQUID WASTE STREAM.

DESCRIPTION:

This system consists of a light tight detector assembly which is interfaced with the sample via male 1/8" pipe fittings with the readout and processor assembly via two BNC connectors.

The sample is passed through a filter and thence to the detector assembly, where it is viewed by two pairs of matched photo multiplier tubes.

The table top or rack mounted processor and display portion of this system conditions and analyzes the output from the photo multiplier tubes by pulse height and validated by a coincidence circuit, thereby permitting the system to eliminate counting most background (noise) counts.

MEETS CFR/NRC REGULATION OF 1.0 $\mu\text{Ci/L}$ (H-3)

NexTritium-H₂O includes unique statistical Significance Display.

- This function rates strength of the data preventing most false positives or negatives:
 - Significance : **HIGH, LOW, or NOT SIGNIFICANT.**



TECHNICAL ASSOCIATES

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303

PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@TECH-ASSOCIATES.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISION OF



07C08-UCLC

AUTOMATED LOW-LEVEL TRITIUM IN WATER MONITOR REAL TIME CONTINUOUS

Model ~ NexTritium-H₂O

UNIQUE NEXTRITIUM-H₂O DETECTOR CHARACTERISTICS

FEATURE	PURPOSE
Ultra High Sensitivity Achieved Through the Following Physical Features:	
Custom Made Anthracene Scintillation Crystals in Technical Associates' Laboratories	High Beta Sensitivity
Two (2) 5" Diameter Optical Sensor Arrays (Totaling 200 cm ²) Sensitive Area	High Count Rate
Special Data Analysis	As Described in Sensitivity Chart
Guard Detector	Cosmic Ray Rejection
Four (4) Photo Sensors	True Tritium Pulse Validation
Five (5) Flow Channels	Assures Smooth Continuous Flow
Temperature Controlled Detector Cooler	Long Term Accurate Signal Stability
Steel, Bronze, and Lead Shielding	Gamma Ray Background Rejection
Real-Time Temperature Compensation Sensor	Improved Sensitivity & Stability



TECHNICAL ASSOCIATES

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303

PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@TECH-ASSOCIATES.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISION OF



USNUCLEARCORP

OTCQB-UCLC

AUTOMATED LOW-LEVEL TRITIUM IN WATER MONITOR REAL TIME CONTINUOUS

Model ~ NexTritium-H₂O

TRITIUM SENSITIVITY		
PicoCuries	MicroCuries	Time to Count
2,000,000 pCi/l	2.0 μ Ci/l	2 minutes
500,000 pCi/l	0.5 μ Ci/l	20 minutes
200,000 pCi/l	0.2 μ Ci/l	3 hours
100,000 pCi/l	0.1 μ Ci/l	24 hours
20,000 pCi/l	0.02 μ Ci/l	7 days
10,000 pCi/l	0.01 μ Ci/l	14 days
Display updates every 2 minutes		

FLOW CHART

1. Chiller
2. Refrigerated Detector & Amplifiers to Sustain Constant Low Temperature
3. Flow Cell – 5" Diameter
4. Photo Multiplier Tube
5. Guard Detector

FEATURES OF SENSOR SYSTEM

- Real-Time Temperature Detection & Correction
- Real-Time Dynamic Gamma Background Detector.



TECHNICAL ASSOCIATES

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303

PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@TECH-ASSOCIATES.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISION OF



USNUCLEARCORP

OTCQB-UCLF

AUTOMATED LOW-LEVEL TRITIUM IN WATER MONITOR REAL TIME CONTINUOUS

Model ~ NexTritium-H₂O

SPECIFICATIONS:

Display Update:	Every 2 minutes.
Tritium Sensitivity:	See Tritium Sensitivity Chart above
Range:	20,000 - 20,000,000 pCi/liter Optional : Other ranges higher or lower.
Flow Rate:	Minimum -1 ml/min
Maximum -	100 ml/min
Sample Temperature: Standard -	< 80°F (liquid); (optional - to 115°F)
Ambient Temperature:	Detector - < 80°F (Optional - to 115°F) Readout-< 115°F
Lead Shielding:	1" thick is standard 2" thick is optional

WEIGHT & DIMENSIONS:

Dimensions:	Electronics: 23"H x 16"L x 21" W (58.4 cm x 40.6 cm x 53 cm) Detector: 12"H x 10"D x 27" W (30.4 cm x 25.4 cm x 68.6 cm) Pump: 10"H x 10"D x 6" W (25.4 x 25.4 cm x 16 cm)
Weight (Standard Unit):	Detector Housing: 35 lbs. (Unshielded) (15.8 kg) Electronics Housing: 40 lbs.(18 kg) Pump: 8 lbs (3.6 kg)
Shipping Weight:	90 lbs.

➤ **Weight and Dimensions shown above do not include Sample Chiller and Refrigeration Unit.**

Optional Shielding:	65 lbs. (29 kg)
Display:	5" color monitor (12.7 cm)

OPTIONS

- Data Archive and Data Retrieval; records readings for up to 5 years.
- Remote readout via Ethernet
- Network reporting and communication via the ORO overdrive network
- "Deionizer and Filter" specification (SSS-33M8/D and SSS-33M8/F).



TECHNICAL ASSOCIATES

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303

PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@TECH-ASSOCIATES.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISION OF




USNUCLEARCORP

OTCQB-UCLC

AUTOMATED LOW-LEVEL TRITIUM IN WATER MONITOR REAL TIME CONTINUOUS

Model ~ NexTritium-H₂O

NexTritium-H₂O FLOW CHART

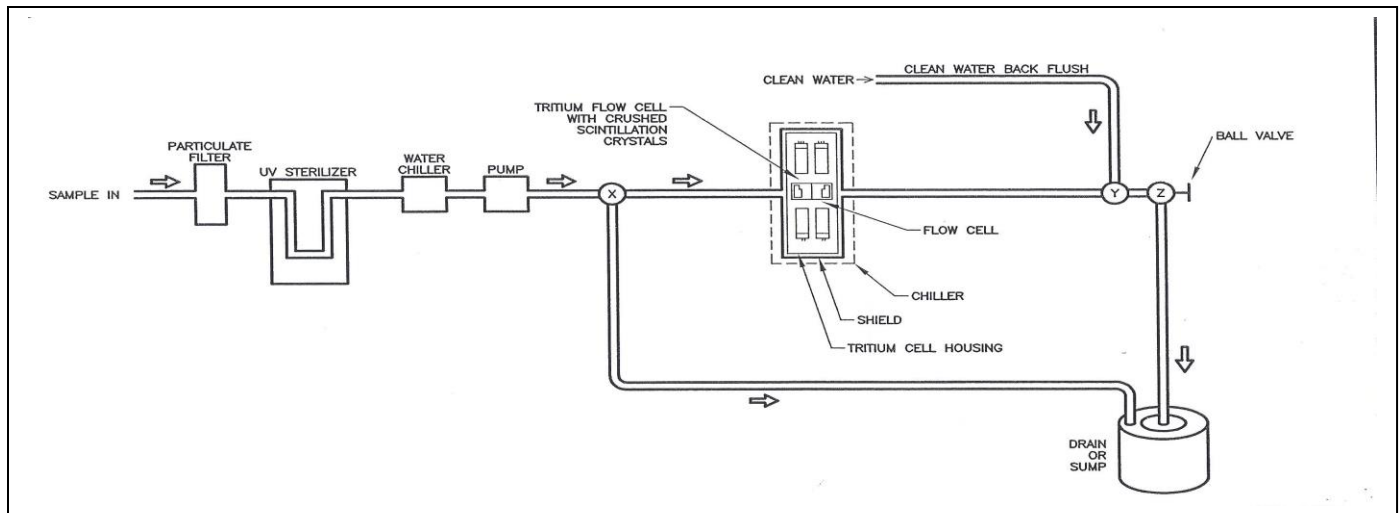

IF YOU HAVE TRITIUM IN WATER & OIL MIXTURES: WE RECOMMEND THIS STRATEGY FOR MEASUREMENT OF TRITIUM

STRATEGY

Tritium is radioactive hydrogen, and hydrogen atoms regularly jump or exchange between different adjacent molecules.

In a mixture of normal water mixed with tritiated oil, both components will, over time, share the Tritium equally.

In **LIQUID** Samples, this allows a separation strategy, in which we,

1. Pull a sample from the mixture
2. Run this sample through a oil-water separator
3. Collect the relatively clean water
4. Pull this water into the SSS-33M81 tritium measurement flow cell
5. Get a good reading
6. Without contaminating or degrading the cell

In **GASEOUS** Samples, the same principles apply.

1. A vapor separation system is utilized.
2. A [PTG-9](#) Tritium Measurement Ion Chamber is used to make the measurements.

**PLEASE CONTACT US WITH INFORMATION ON YOUR SITUATION.
WE WILL ADVISE &/OR QUOTE ON A SUITABLE SYSTEM TO OBTAIN YOUR OBJECTIVE.**



TECHNICAL ASSOCIATES

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303

PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@TECH-ASSOCIATES.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISION OF
 USNUCLEARCORP
OTCQB-UCLF